

TEST REPORT

(Electronic version)



No:200058912

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: TYEJ-0990-04

ISSUE DATE:2020-04-15

检测报告



APPLICANT: DONGGUAN MAGICING INFORMATION TECHNOLOGY CO,LTD
ADDRESS: NO.20,QINANQIULING 1STSTREET,TIESONG VILLAGE ,QINGXI ,DONGGUAN CITY

INFORMATION CONFIRMED BY APPLICANT:

KN95 MASK

QUANTITY: FIFTY PIECES

DATE RECEIVED/DATE TEST STARTED: 2020-04-15

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"----" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200062574.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

Yuan Liu ENGINEER

刘 圆




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200058912

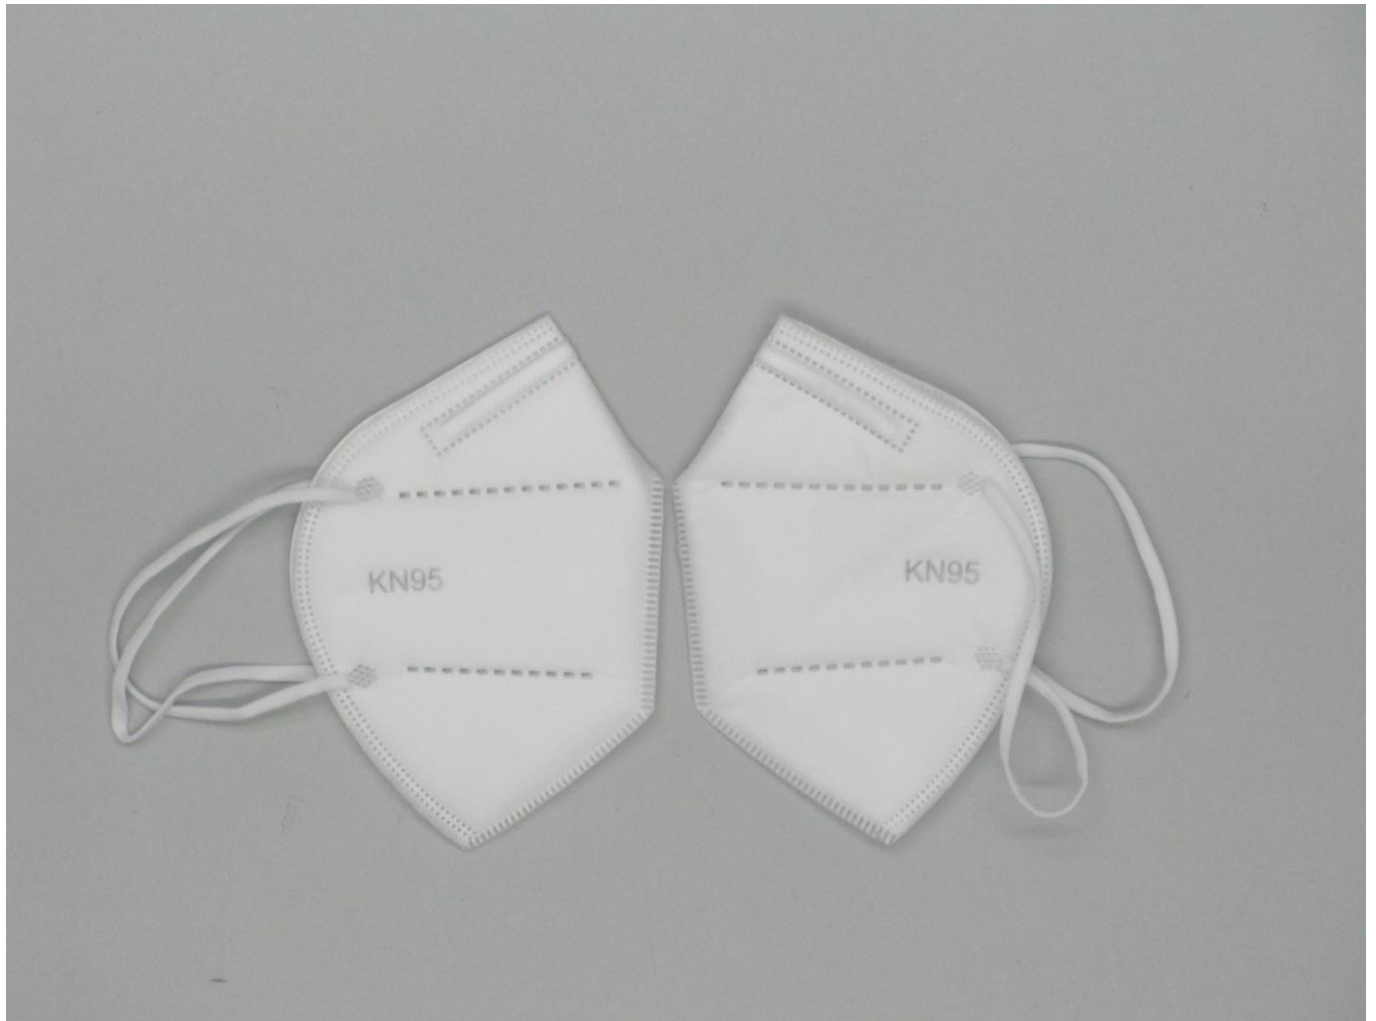

TEST REPORT

(Electronic version)

No:200058912

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³,
TEMP:23.0℃, RH:36.1%)

FILTRATION EFFICIENCY(%) :

UNTREATED SAMPLE

1# 98.87
2# 98.76
3# 99.011
4# 99.048
5# 98.90
6# 98.97
7# 98.56
8# 98.71
9# 99.142
10# 98.69

CONDITIONING TREATED

1# 97.04
2# 97.28
3# 96.89
4# 97.11
5# 96.95

REQUIREMENT

FILTRATION EFFICIENCY(%) :

≥95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 134.2
2# 131.1

PRETREATMENT SAMPLE:

1# 118.7
2# 112.6

REQUIREMENT

≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 103.4
2# 104.7

PRETREATMENT SAMPLE:

1# 104.8
2# 100.3

REQUIREMENT

≤250
(GB 2626-2006)

FLAMMABILITY (s)

(GB 2626-2006 6.15)

AFTERFLAME TIME

UNTREATED SAMPLE

1# 0.0
2# 0.0

CONDITIONING TREATED

3# 0.0
4# 0.0

REQUIREMENT

AFTERFLAME TIME
≤5
(GB 2626-2006)



PAGE 3 OF 4



中国认可
国际互认
检测
TESTING
CNAS L10314

TEST REPORT

(Electronic version)

No:200058912

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST
PARTS OF MASK SHOULD NOT SLIP OR BREAK
UNDER 10N TENSION FOR 10S.

(GB 2626-2006)



——End of Report——

PAGE 4 OF 4